

Figure 1

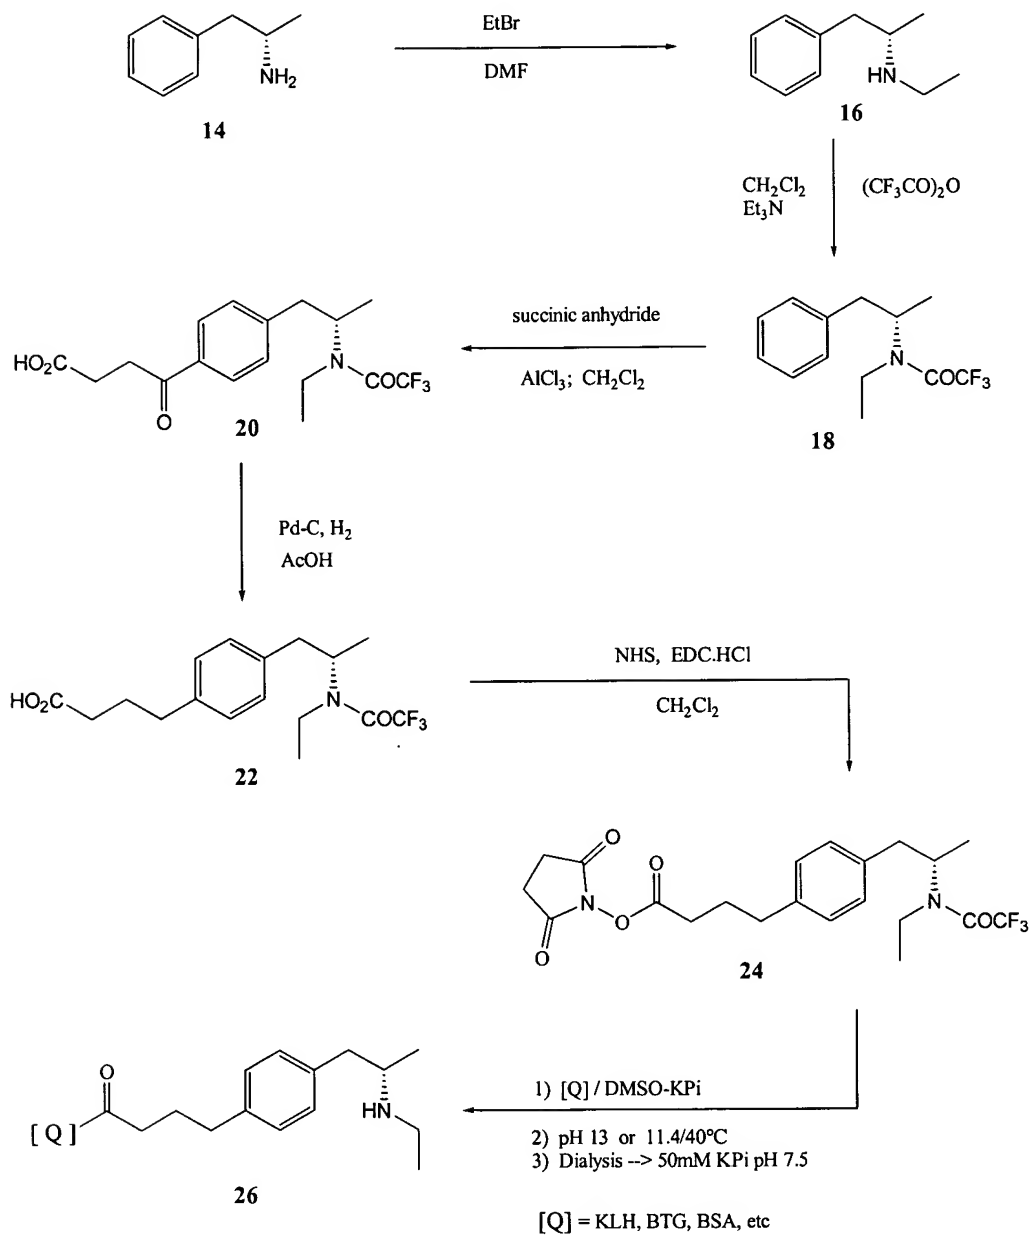


Figure 2

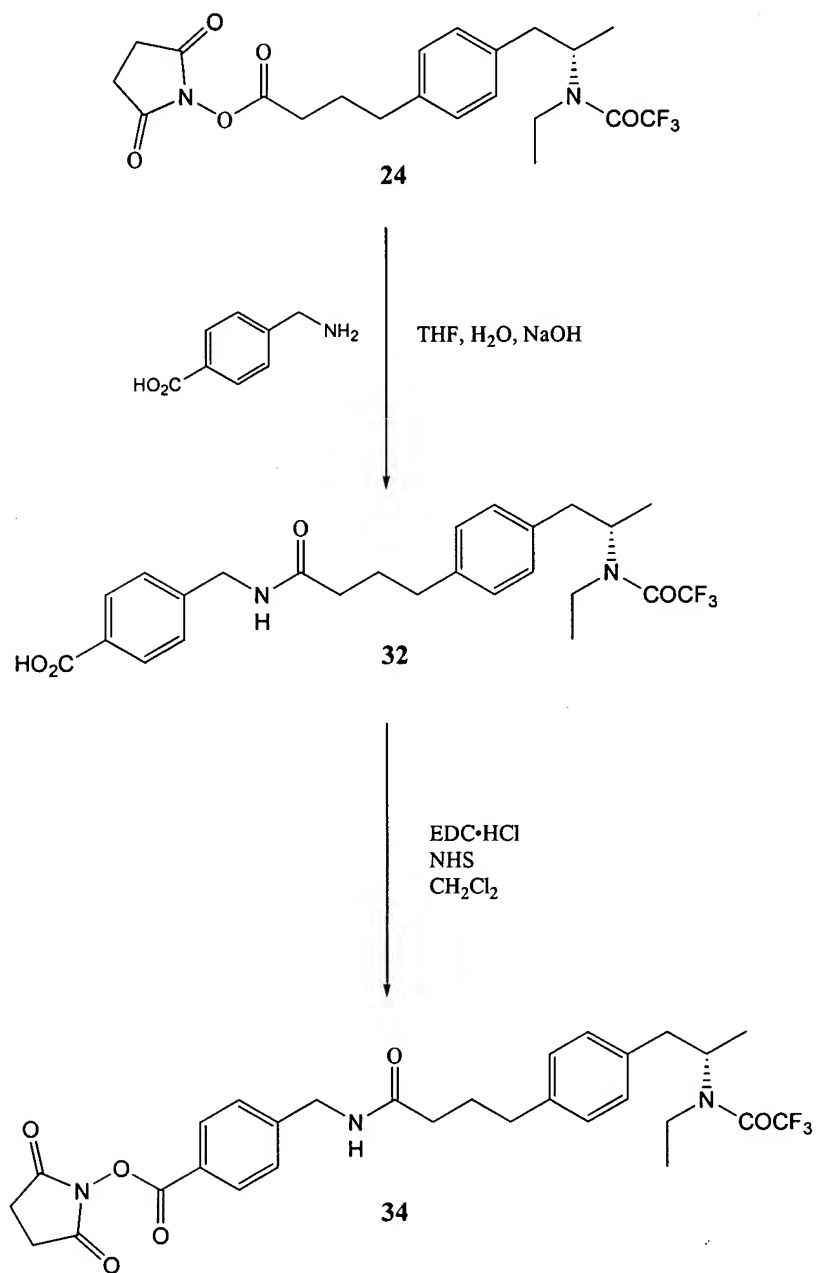


Figure 3

Calibration curve using antibody MDMA 2.1.1

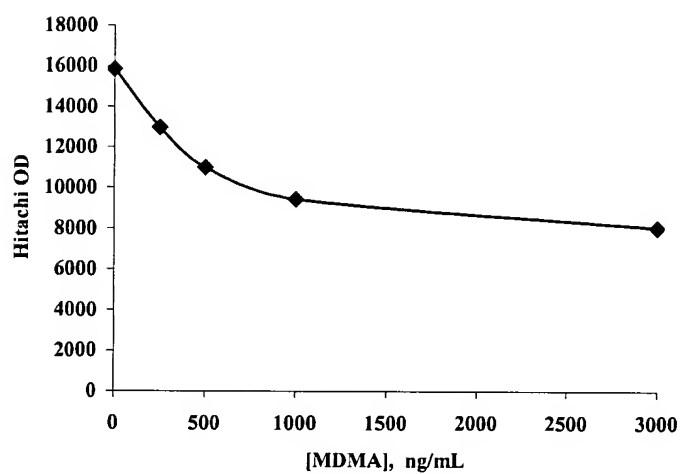


Figure 4

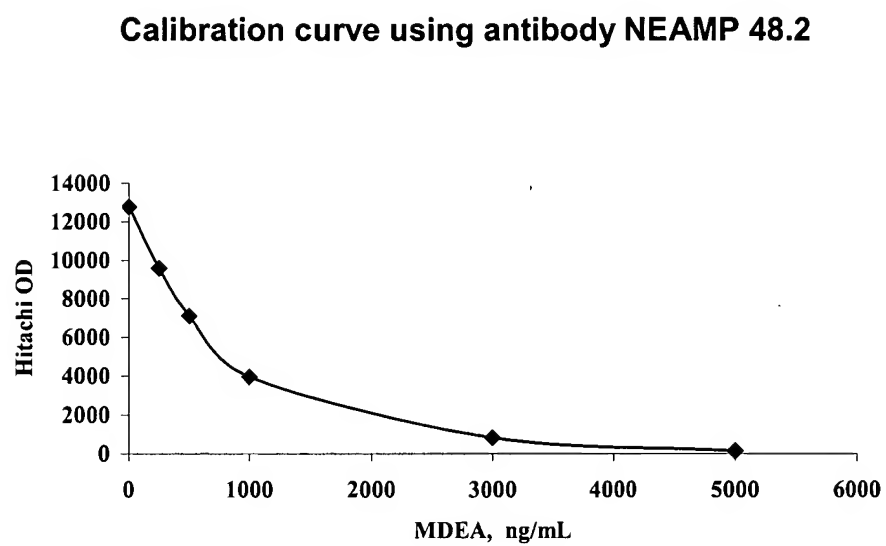


Figure 5

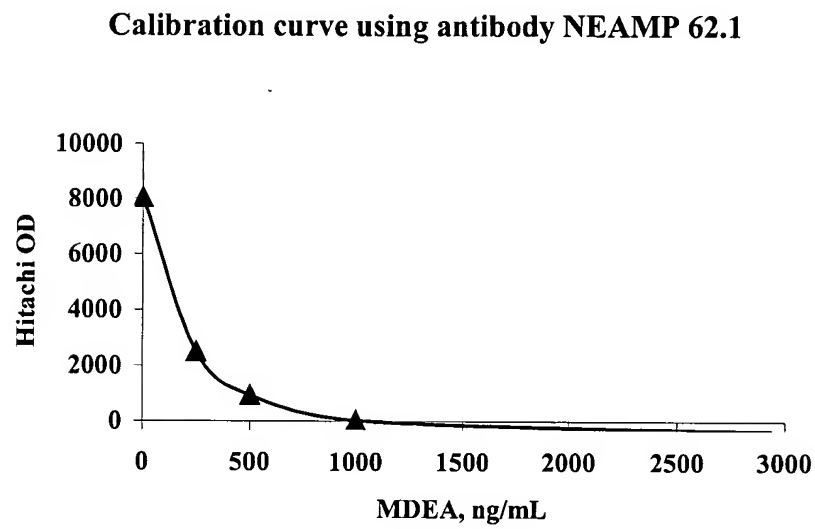


Figure 6